

## Medipac 2000 Standard Medipac 2000 Superplus Midi (Type 0035 to 0100)

Complete purification package including adsorption dryer, activated carbon adsorber, pre-, afterfilter and condensate drain

The Medipac 2000 breathing air systems are purification units based on adsorption dryers Ultrapac 2000 to supply breathing air in excess of all relevant international standards and medical prescriptions.

The purification consists of several stages:

Compressed air is led through the inlet of the unit (J) and across the pre filter (2). At this stage, the air is cleaned from particles and condensate. The condensate is removed via a membrane condensate drain (5). The following desiccant dryer reduces the water vapour content of the compressed air down to a pressure dew point of  $-40^{\circ}\text{C}$  (equivalent to a remaining water content of  $0.11 \text{ g/m}^3$ ). In the following purification stages (SP, AK, OX) (9) the content of  $\text{CO}_2$  is adsorbed to a level far below 500 ppm the content of  $\text{SO}_2$  below 1 ppm and the content of  $\text{NO}_x$  below 2 ppm. In the AK stage oil vapours, hydrocarbons, taste and odours are adsorbed to a level far below  $0.003 \text{ mg/m}^3$ . In the OX stage a catalyst converts CO to  $\text{CO}_2$  and thereby reduces the carbon monoxide level down below 5 ppm.


The final particle filter (3) removes all particles which might be carried over from the adsorption and /or catalyst stages.



**Medipac 2000  
Superplus**

Medipac 2000	Volume flow in $\text{m}^3/\text{h}$ (1 bar, $20^{\circ}\text{C}$ )*	Reg. air flow average $\text{m}^3/\text{h}$ (1 bar, $20^{\circ}\text{C}$ )	Volume flow out (min.) $\text{m}^3/\text{h}$ (1 bar, $20^{\circ}\text{C}$ )	Pressure loss initial mbar
0035	35	5.95	27.6	95
0050	50	8.5	39.4	120
0065	65	11.05	51.2	155
0080	80	13.6	63.0	280
0100	100	17	78.8	450

\* Related to 1 bar (abs) and  $20^{\circ}\text{C}$  at intake of compressor and 7 bar (g) and  $35^{\circ}\text{C}$  inlet temperature

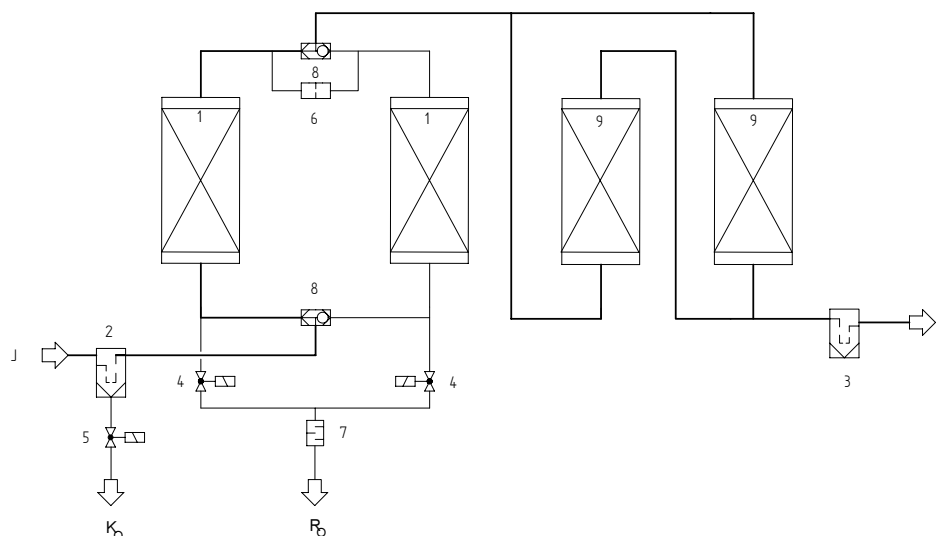

## Medipac 2000 Standard Midi / Superplus Midi

Features Medipac 2000:	Benefits:
Purification package including adsorption dryer, CO-, CO <sub>2</sub> -, NO <sub>x</sub> - and SO <sub>2</sub> removal, pre-, afterfilter and automatic condensate drain	Turnkey system, no additional installation costs; all components from one hand, therefore perfect technical match
Guaranteed and validated separation efficiency	Breathing air quality in excess of all relevant international standards, as e.g. Pharmacopée Européenne; DIN EN 12021 (DIN 3188); EN 737-3; BS4275; ANSI/CGA G.7.1; Z180, 1 M85; AS2299-1979; NZL5813
Adsorbent in cartridges	Easy storage, transport and installation; optimum fixation of desiccant; no risk of fluidizing of desiccant
Compact, space saving design	Installation in smallest spaces, possible also as retrofit
Component exchange display	High operating safety, due to calculation of optimum exchange point for filter elements and desiccant cartridges
Unique Multifunction Block	All moving parts and all electronic components integrated in a function block, therefore easy and efficient maintenance

Features Medipac 2000 Superplus:	Benefits:
Intermittent operation standard	Link between dryer and compressor possible on central applications, therefore saving of regeneration air
Load dependent control	Adjustment of adsorption cycles to the actual inlet water load, therefore saving of regeneration air and reduction of operating cost
Self-Diagnosis-System	Sensor-controlled monitoring of regeneration air flow, therefore without-gap-monitoring of dryer functions and of system pressure
Text Display	Display of all operating status, of fault indication and maintenance intervals in clear text messages
Info-Channel	Serial interface for transmission of alarm- and maintenance messages
Economizer-Function	Online calculation of optimum exchange point of filter elements by continuous evaluation of energy cost versus cost of replacement filter element

**Sizing:**

f	4 bar(g)	5 bar(g)	6 bar(g)	7 bar(g)	8 bar(g)	9 bar(g)	10 bar(g)	11 bar(g)	12 bar(g)	13 bar(g)	14 bar(g)	15 bar(g)	16 bar(g)
25°C	0.69	0.82	0.96	1.10	1.24	1.38	1.50	1.50	1.50	1.50	1.50	1.50	1.50
30°C	0.69	0.82	0.96	1.10	1.24	1.38	1.50	1.50	1.50	1.50	1.50	1.50	1.50
35°C	0.63	0.75	0.88	1.00	1.13	1.26	1.38	1.50	1.50	1.50	1.50	1.50	1.50
40°C	0.48	0.58	0.68	0.77	0.87	0.96	1.06	1.16	1.25	1.35	1.45	1.50	1.50
45°C	0.38	0.45	0.53	0.60	0.68	0.75	0.83	0.90	0.98	1.05	1.13	1.20	1.28
50°C	0.30	0.36	0.42	0.48	0.54	0.60	0.66	0.72	0.78	0.84	0.90	0.96	1.02

$$\dot{V}_{corr} = \frac{\dot{V}_{nom}}{f}$$
 Example:  $\dot{V}_{nom} = 50 \text{ m}^3/\text{h}$ , Inlet temperature = 30°C, Operating pressure = 10 bar (g)

$$\dot{V}_{corr} = \frac{50 \text{ m}^3/\text{h}}{1.50} = 33,33 \text{ m}^3/\text{h}$$
 Calculated dryer size: Medipac 2000, type 0035

Product description:
<b>Medipac 2000 Standard and Superplus:</b> Complete purification package including adsorption dryer, CO-, CO <sub>2</sub> -, NO <sub>x</sub> - and SO <sub>2</sub> removal, pre-, afterfilter and automatic condensate drain

Medium:
Compressed air

Operation pressure:
min. 4 bar (g), max. 16 bar (g)

Medium temperature:
min. 5 °C, max. 50 °C

Ambient temperature:
min. 4 °C, max. 50 °C

Compressed air consumption:
17% of the rated flow, in average


Power supply:
230 V/50 -60 Hz AC; 110 V/50 -60 Hz AC 24 V DC; 24 V AC on request

Power consumption:
approx. 4 W

Air quality related to standard inlet conditions:	
Particles	< 1 µm
Residual oil content	< 0.01 mg/m <sup>3</sup>
Oil vapour and hydrocarbons	< 0.003 mg/m <sup>3</sup>
Water vapour	PDP - 40°C (= 0.11 g/m <sup>3</sup> )
CO <sub>2</sub>	< 500 ppm
CO	< 5 ppm
SO <sub>2</sub>	< 1 ppm
NO <sub>x</sub>	< 2 ppm
Taste and odours	taste and odour free

Declaration of conformity:
acc. to 73/23/EC 97/23/EC

## Medipac 2000 Standard Midi Medipac 2000 Superplus Midi

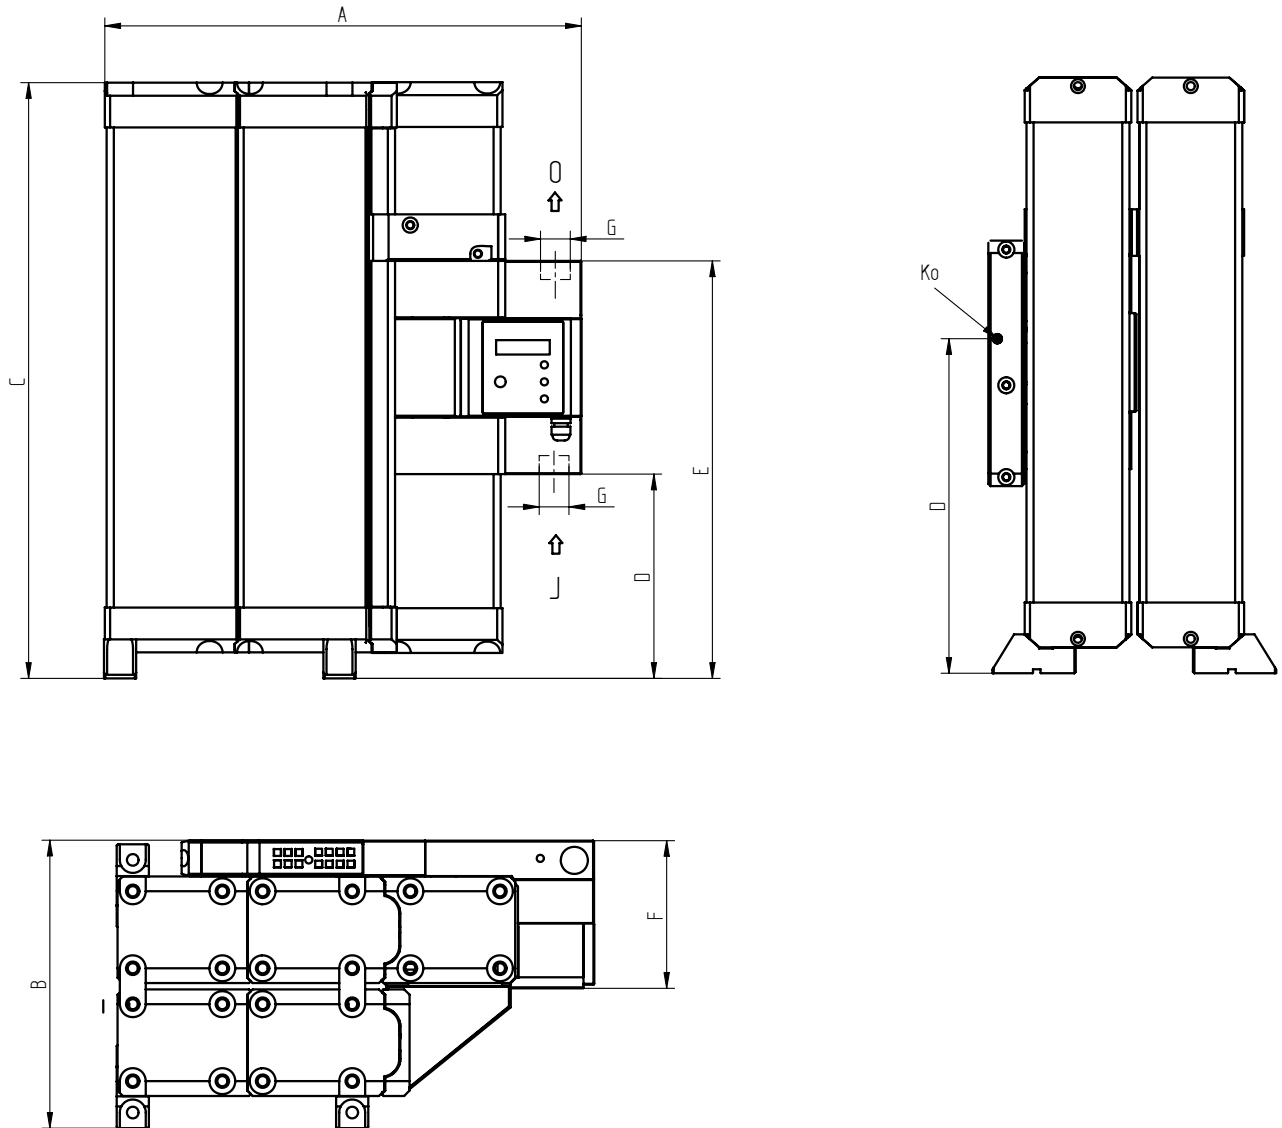

Medipac 2000 Midi							
Type	G "	A mm	B mm	C mm	D mm	E mm	F mm
0035	G 1	532	322	665	230	465	165
0050	G 1	532	322	920	355	595	165
0065	G 1	532	322	1170	485	720	165
0080	G 1	532	322	1420	605	845	165
0100	G 1	532	322	1670	730	970	165